



# ScanCast™ Action Barcodes:


Meditech Formulary Meditech Formulary [SCRXMTDFSCRXMTDF]  
Large (3x3)

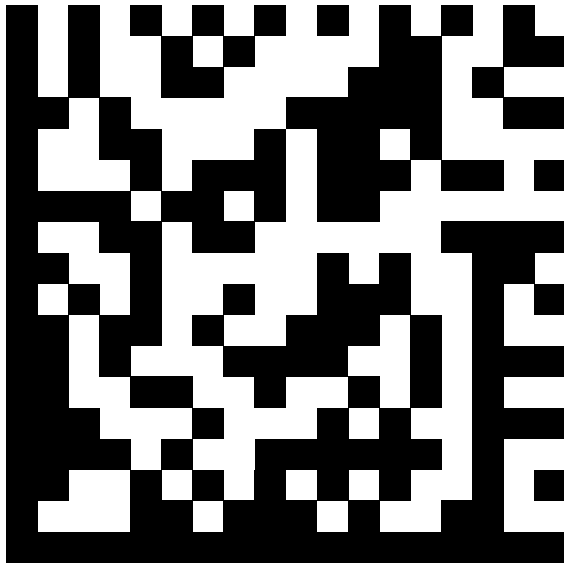


Reset

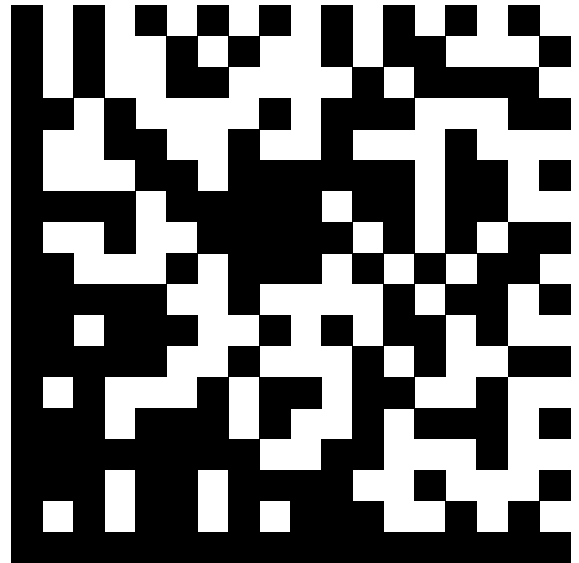

Enable <sup>[1]</sup>

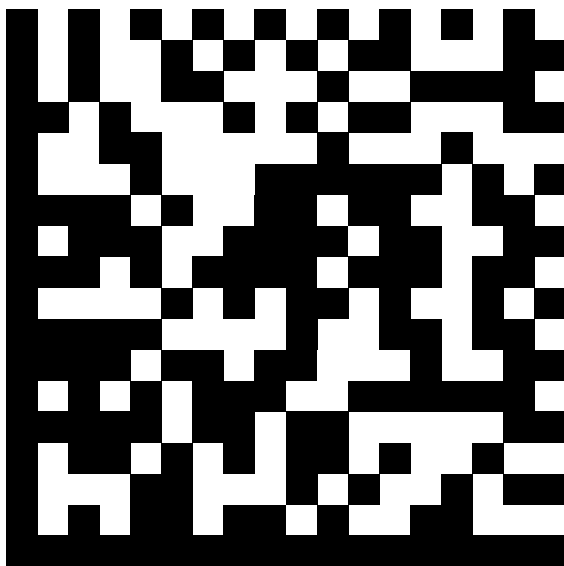

Disable

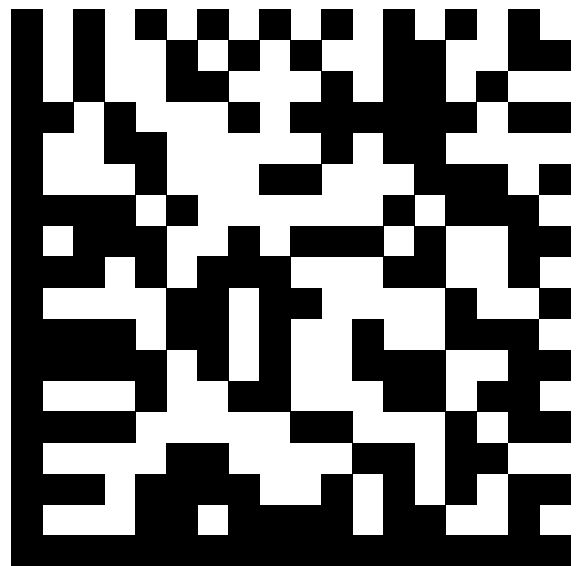

Fail


[1] Default setting at power on

[2] Non-volatile setting, shall be retained across power cycle




# ScanCast™ Action Barcodes:

Meditech Formulary Meditech Formulary [SCRXMTDFSCRXMTDF]  
Large (3x3)

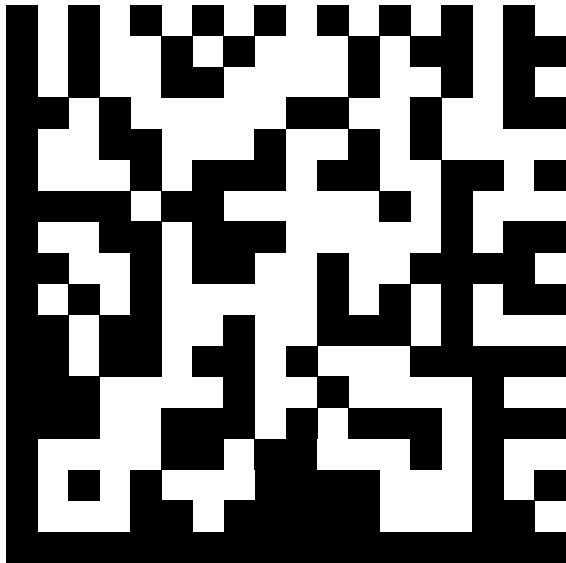

Mode 0 [2]

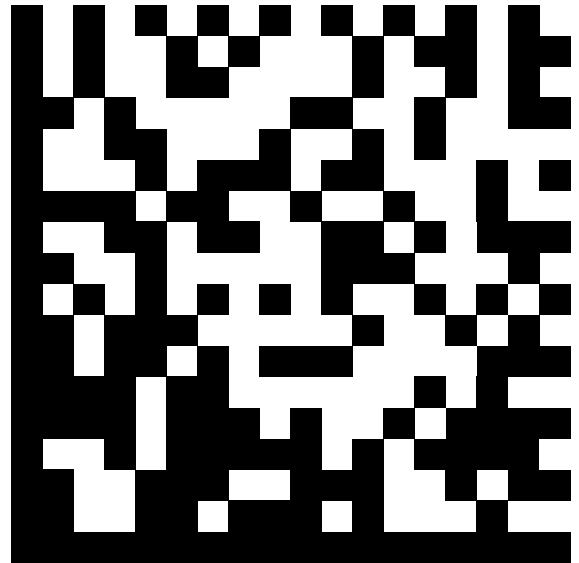

Mode 1 [2]

[1] Default setting at power on

[2] Non-volatile setting, shall be retained across power cycle