



ScanCast™ Action Barcodes:


Meditech Formulary Meditech Formulary [SCRXMTDFSCRXMTDF]
Medium (1.75x1.75)

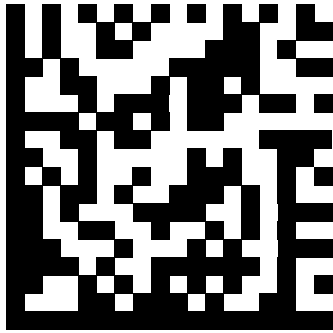


Reset

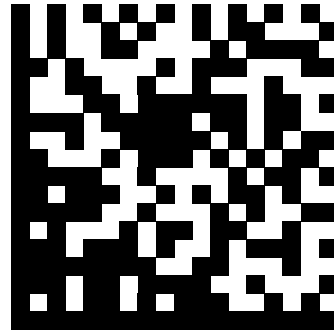


Enable ^[1]

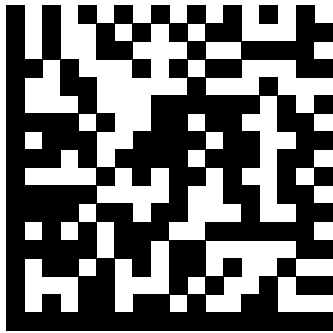


Disable

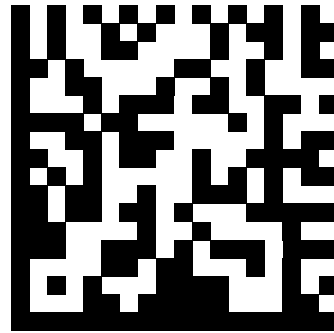

Mode 0 ^[2]

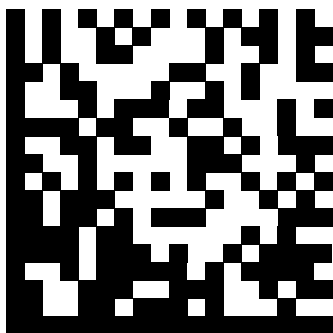

Mode 1 ^[2]

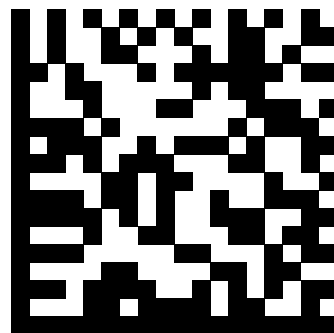

Fail

[1] Default setting at power on

[2] Non-volatile setting, shall be retained across power cycle